


Latex Blue with NEU-THERA®

Sterile
Emollient Coating



A smart foundation

- Ideal **underglove** when double-gloving
- Distinct **blue color** aids in alerting wearers to perforations in the outer glove⁴
- **NEU-THERA®** Emollient Coating aids in wet and dry donning, helps promote **skin moisturization** and supports **hand hygiene** compliance⁵
- Interlocking, beaded cuff design helps to **prevent roll-down**
- Proprietary hand mold with an independent thumb design allows for an **anatomical fit and natural movement**

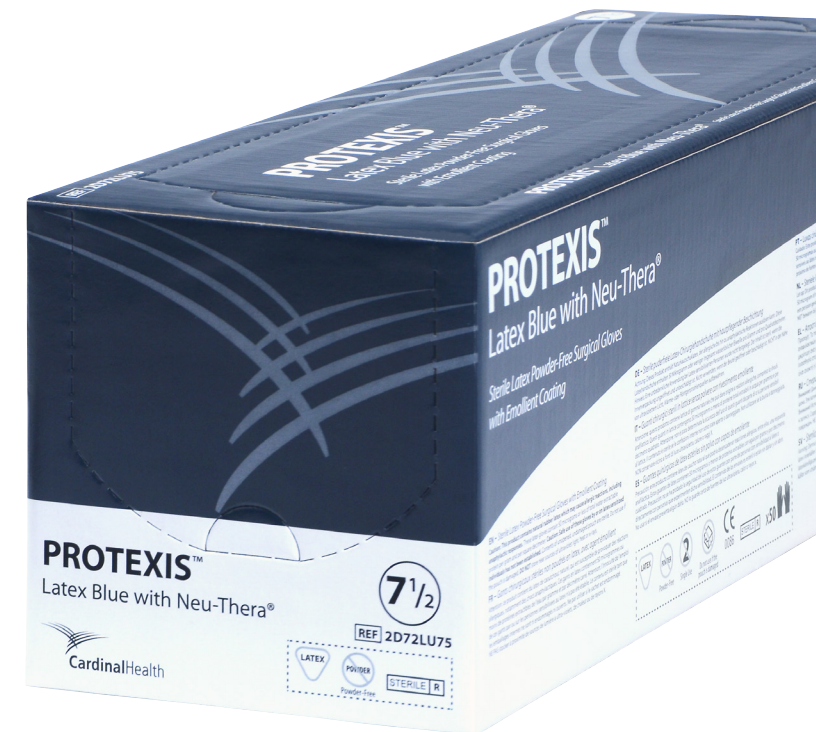



Backed by the expertise of Cardinal Health, PROTEXIS™ Latex Blue with NEU-THERA® Surgical Gloves meet all relevant FDA and ASTM standards, including those for physical dimensions⁶, physical properties⁶ and freedom from holes⁷. Documentation is available upon request.

PROTEXIS™ Latex Blue with NEU-THERA® Surgical Gloves are an ideal base layer in a double-gloving system. The NEU-THERA® Emollient Coating moisturizes and soothes the skin⁵, while their blue color helps alert the wearer to potentially dangerous perforations.⁴

Properties (before aging)

| | |
|-------------------------------------|--------------------------|
| Tensile strength | Min 24 MPa ⁶ |
| Stress at 500% elongation (modulus) | Max 5.5 MPa ⁶ |
| Ultimate elongation (elasticity) | Min 750% ⁶ |
| Puncture resistance (cuff) | Min 5N ⁸ |
| Freedom from holes ⁷ | 0.65 AQL ⁶ |



| Catalog no. | Size | Length | Thickness ⁶ | | | Material | Color | Cuff type | Protein content | Qty/ bx | Qty/ cs |
|-------------|------|---------------------|------------------------|---------------------|---------------------|--|---|-------------------|---------------------------------|---------|---------|
| | | | Finger | Palm | Cuff | | | | | | |
| 2D72LU55 | 5.5 | 11.1 in./ 282 mm | 7.5 mil/ 0.19 mm | 5.5 mil/ 0.14 mm | 5.5 mil/ 0.14 mm | Natural rubber latex with nitrile polymer and Neu-Thera® Emollient Coating |  Blue | Beaded/ Rolled | Less than 50 µg/dm ² | 50 | 200 |
| 2D72LU60 | 6 | | | | | | | | | | |
| 2D72LU65 | 6.5 | | | | | | | | | | |
| 2D72LU70 | 7 | 11.6 in./ 295 mm | 7.5 mil/ 0.19 mm | 5.5 mil/ 0.14 mm | 5.5 mil/ 0.14 mm | Natural rubber latex with nitrile polymer and Neu-Thera® Emollient Coating |  Blue | Beaded/ Rolled | Less than 50 µg/dm ² | 50 | 200 |
| 2D72LU75 | 7.5 | | | | | | | | | | |
| 2D72LU80 | 8 | | | | | | | | | | |
| 2D72LU85 | 8.5 | | | | | | | | | | |
| 2D72LU90 | 9 | | | | | | | | | | |

1 Tested in accordance with ASTM D 5712

2 Tested in accordance with ASTM D 6124

3 Caution: This product contains natural rubber latex which may cause allergic reactions.

4 77% of perforations can be detected with an indicator under the gloves, compared with only 21 percent in standard double-gloving, and even fewer with single-glove technique. Waljee J, Malay S, Chung K. Sharps Injuries: The Risks and Relevance to Plastic Surgeons. *Plast. Reconstr. Surg.* 131: 784, 2013.

5 Data on file with Cardinal Health. California Skin Research Institute Study, Project Number 03-118.

6 In accordance with ASTM D 3577

7 Tested in accordance with ASTM D 5151

8 Tested in accordance with AS/NZS 4179, average test result = 8.4N

9 35% reduction of materials used as compared to previous Cardinal Health packaging design. Cardinal Health Technical Council Conference 2011, presentation on file.

The Cardinal Health™ PROTEXIS™ Surgical Gloves promise:

We protect so you can perform.

As a leader in the industry with more than 50 years of surgical gloves experience, Cardinal Health is dedicated to providing protection, performance and expertise so wearers can perform confidently and focus on their patients.



Help maximize storage space: Half-fold packaging design reduces packaging material⁹



Storage recommendations: It is recommended that gloves are properly stored away from light and extreme temperatures. Gloves should also be protected from direct exposure to ozone-generated devices such as fluorescent lights, electrical motors and x-ray devices.



Expiration: 35 months from date of manufacture. Expiration date is printed on packaging.



CardinalHealth™

cardinalhealth.com/surgicalgloves

GMB-CAH-ProductSupport@cardinalhealth.com

Customer service: 800.964.5227

© 2019 Cardinal Health. All Rights Reserved. CARDINAL HEALTH, the Cardinal Health LOGO, and PROTEXIS are trademarks of Cardinal Health and may be registered in the US and/or in other countries. Lit. No. 2MS19-1042514-1(12/2019)