


Patterson Medical Alarm Monitors

Patterson Medical (US and Canada)
 Economy **0815-62-537**
 Standard **0815-61-497**
 Deluxe **0815-61-505**

Patterson Medical, Ltd.
 Economy **09 151 4496**
 Standard **09 151 4504**
 Deluxe **09 151 4512**

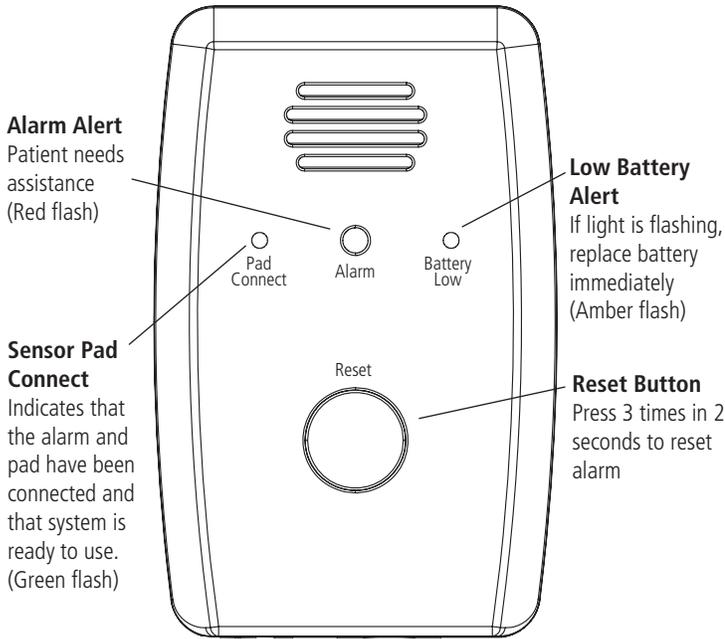

Before First Setup

Inspect monitor and components closely. If damage is spotted, contact us immediately. Designed for use with Patterson Medical sensor pads.

Please read all instructions for alarm monitor and sensor pad. If they are not clear, consult a medical professional. Failure to follow instructions, precautions and warnings could damage equipment and/or result in injury to the patient.

Monitor Features



Familiarize yourself with the monitor features of each model (refer to illustrations). Look for the feature controls on the following locations:

On the front of the monitor: Reset Button and LED indicators for Low Battery, Alarm and Connect Pad.

On the bottom: Nurse Call Cord Jack, Sensor Pad Jack, AC Adapter Power Jack.

Inside battery compartment: Volume Control (Hi/Lo/Silent), Tone Switch, Delay Switch (0/1 sec/2 sec), Record Button, Nurse Call (NC/NO).

(Instructions on back)

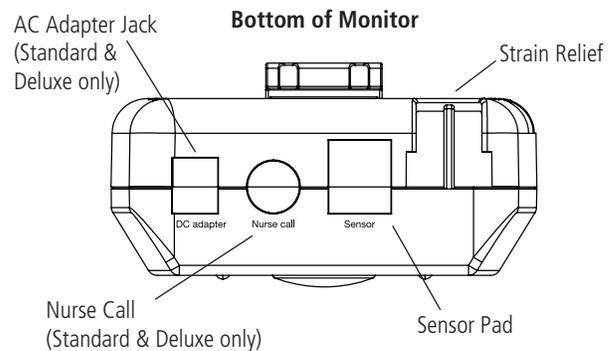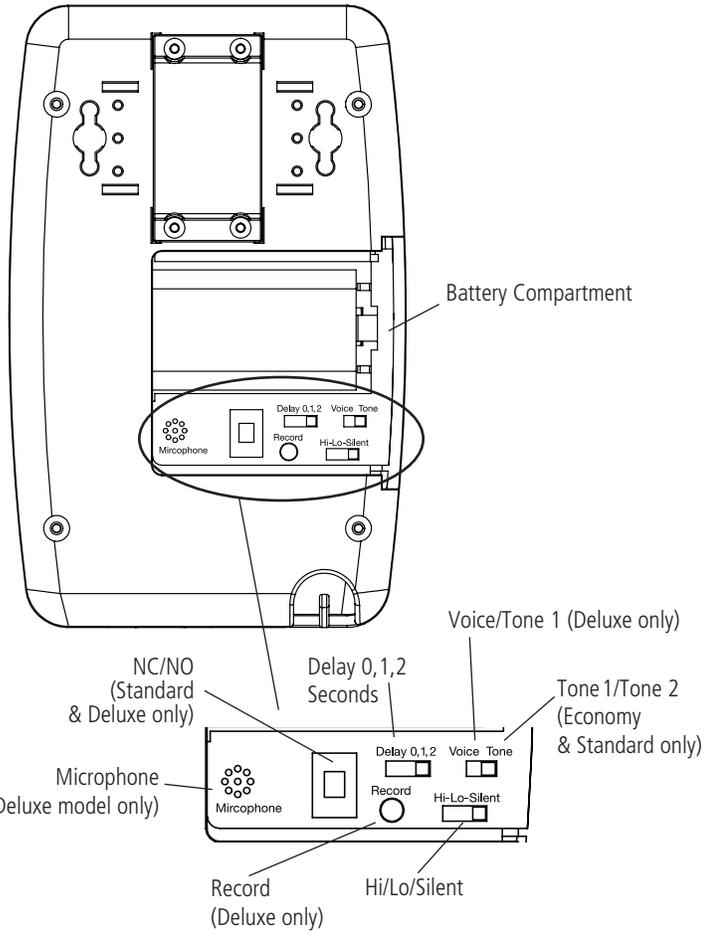

Distributed by:
Patterson Medical
 28100 Torch Parkway, Ste. 700
 Warrenville, IL 60555, USA
 Phone: 800-323-5547
 Direct Phone: 630-393-6000
 Fax: 800-547-4333
 Direct Fax: 630-393-7600

Patterson Medical
 W68 N158 Evergreen Blvd.
 Cedarburg, WI 53012, USA
 Phone: 800-323-5547
 Fax: 800-547-4333

Patterson Medical Canada
 6675 Millcreek Drive, Unit 3
 Mississauga, ON L5N 5M4
 Phone: 800-665-9200
 Direct Phone: 905-858-6000
 Direct Fax: 905-858-6001
 Toll-Free Fax: 877-566-8611

Authorized European Representative
Patterson Medical, Ltd.
 Nunn Brook Road
 Huthwaite, Sutton-in-Ashfield
 Nottinghamshire, NG17 2HU, UK
International
 Phone: +44 (0) 1623 448 706
 Fax: +44 (0) 1623 448 784

| Description | Pad Connect LED Indicator | Alarm LED Indicator | Low Battery LED Indicator | Reset Button | Hi/Lo/Silent Switch | 0/1sec/2sec Delay Switch | Tone Switch | Voice Record | Nurse Call Jack | AC Adapter Interface |
|------------------------|---------------------------|---------------------|---------------------------|--------------|---------------------|--------------------------|-------------|--------------|-----------------|----------------------|
| Economy Alarm Monitor | X | X | X | X | X | X | X | | | |
| Standard Alarm Monitor | X | X | X | X | X | X | X | | X | X |
| Deluxe Alarm Monitor | X | X | X | X | X | X | X | X | X | X |

Precautions

The monitor and sensor pad are NOT A SUBSTITUTE for visual monitoring. The system DOES alert caregivers of potential risks, but it DOES NOT prevent falls. The monitor also indicates when a patient needs assistance.

Use the system as part of your overall fall protection program, and set up protocols such as logging the date the sensor pad is first used. This date should be indicated on the pad itself and in patient's records. If someone else uses the sensor pad, the first date of use should be recorded in that patient's chart.

Assess each patient or resident to determine whether he or she will be uncooperative and possibly thwart the alarm system.

Ensure the monitoring system is working before each use. Double check the instructions for sensor pad such as making sure the pad is flat at all times. Other precautions about sensor pads include the possibility that they have been exposed to moisture and excessive wear and tear on the pads or cords.

Make sure sensor pad air intake ("neck" of chair or over-mattress sensor pad) is clear and not blocked. Air must flow freely in and out of sensor pad for alarm to function. Make sure liquid does not enter at "neck" of sensor pad, as this will damage it. If needed, use an incontinence pad to protect sensor pad from urine or other liquids.

To make the system most effective, respond to alerts immediately.

The sensor pads (and thus the monitor) are not effective for users who weigh less than 70 lbs.

Monitor Setup

Slide the battery compartment to open it, and install the 9V alkaline battery included. Set the volume, tone and delay inside the battery compartment. Once controls are set, slide compartment cover closed until it "snaps" shut.

To attach to wheelchair or bed, thread the chair strap (included) through the bracket on back of monitor.

Connect the sensor pad plug into the Pad Jack on the bottom of monitor. (The alarm will be activated if the sensor pad plug is disconnected from the jack.)

Before each use, test the system. Do this by firmly pressing down on the sensor pad for two seconds. Remove the pressure and the red flash should show on the monitor's indicator, at the same time the alarm tone or voice message should activate.

After testing, reset the monitor by pressing the reset button 3 times within 2 seconds. If possible test the system with the patient sitting or lying on the sensor pad. When pressure is put back on the sensor pad, the alarm signal will automatically go off... as long as the system is working properly. This procedure reminds patient to stay on the sensor pad and alerts the caregiver that there is a risk of patient falling.

Check alerts before and during use:

- Green flash stays on when pad is connected properly. Green flash goes off when pad is lost, not there or faulty.
- Amber flash indicates that battery is low.
- Red flash and alarm tone or recording indicate that the patient has moved off the pad or is standing.

Nurse Call Feature

(Standard and Deluxe Monitor only)

Depending on what nurse call system the facility has (normal close or normal open), the NC or NO switch inside the battery compartment needs to be selected. Simply slide the switch to either one to see which one will work with your nurse call system. Test function of monitor and pad before using with a patient. Use a gentle touch to handle plugs and cords. If cord is pulled too tightly, it can be damaged and cause the system to malfunction.

How to Record Voice Message

(Deluxe Monitor only)

First decide on a message that is less than 15 seconds long. Locate the Record button and Microphone inside the battery compartment. Position the monitor 10" to 12" from your mouth, then press and hold the Record Button; speak

slowly and enunciate words so the message will be clear. Release the button, listen to the message and re-record if necessary.

WARNINGS!

Before each use: check to see if the battery is low. If the low battery light on the front of monitor is flashing, replace 9V alkaline battery immediately. Also verify that mounting clip of the monitor is securely attached to chair or bed.

Only use the Patterson Medical AC Adapter approved for use with this product.

DO NOT immerse monitor or sensor pad in water or liquid. If pad accidentally gets wet, replace immediately.

Inspect the security of the connection at the Nurse Call Jack on the Standard and Deluxe models.

Limited Product Warranty

Patterson Medical warrants that all products shall be free from manufacturing defects for a period of one year from the date of shipment. OTHER THAN THE FOREGOING WARRANTY, PATTERSON MEDICAL MAKES NO REPRESENTATION OR WARRANTY OF ANY KIND, EXPRESS OR IMPLIED, AS TO MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE OR ANY OTHER MATTER RELATING TO THE PRODUCT. Customer must notify Patterson Medical of any manufacturing defect within five days of discovery of the defect. Upon a determination by Patterson Medical that the product is defective, Patterson Medical sole and exclusive obligation shall be to provide customer with a replacement product or a full refund of the purchase price, at the sole discretion of Patterson Medical, and to reimburse customer for any return freight costs. In no event shall Patterson Medical be liable for any other costs or expenses including lost profits or direct, indirect, consequential, incidental or punitive damages. The warranty set forth herein shall govern all purchases, notwithstanding any inconsistent terms and conditions of customer's purchase order.

Optional Accessories

Universal Wide Mounting Bracket
AC Adapter

Chair Sensor Pads

10" x 15" 90-day
10" x 15" 180-day
10" x 15" 1-Year

Bed Sensor Pads

10" x 30" 90-day
10" x 30" 180-day
10" x 30" 1-Year
20" x 30" 90-day
20" x 30" 180-day
20" x 30" 1-Year

Patterson Medical (US and Canada)

0815-61-612
0815-61-620

0815-61-513
0815-61-521
0815-61-539

0815-61-547
0815-61-554
0815-61-562
0815-61-570
0815-61-588
0815-61-596

Patterson Medical, Ltd.

09 151 4520
09 151 4538

09 151 4546
09 151 4553
09 151 4561

09 151 4579
09 151 4587
09 151 4595
09 151 4603
09 151 4611
09 151 4629